

DISPERSIVE LIQUID-LIQUID MICROEXTRACTION BASED ON SOLIDIFICATION OF FLOATING ORGANIC DROP FOR SIMULTANEOUS SEPARATION/PRECONCENTRATION OF NICKEL, COBALT AND COPPER PRIOR TO DETERMINATION BY ELECTROTHERMAL ATOMIC ABSORPTION SPECTROMETRY

Mooud Amirkavei, Shayessteh Dadfarnia* and Ali Mohammad Haji Shabani

Department of Chemistry, Faculty of Science, Yazd University, Yazd, 89195-741, Iran

Recebido em 11/3/12; aceito em 18/7/12; publicado na web em 7/12/12

A dispersive liquid-liquid microextraction based on solidification of floating organic drop for simultaneous extraction of trace amounts of nickel, cobalt and copper followed by their determination with electrothermal atomic absorption spectrometry was developed. 300 μL of acetone and 1-undecanol was injected into an aqueous sample containing diethyldithiocarbamate complexes of metal ions. For a sample volume of 10 mL, enrichment factors of 277, 270 and 300 and detection limits of 1.2, 1.1 and 1 ng L^{-1} for nickel, cobalt and copper were obtained, respectively. The method was applied to the extraction and determination of these metals in different water samples.

Keywords: liquid-liquid microextraction; electrothermal atomic absorption spectrometry; nickel, cobalt and copper determination.

INTRODUCTION

Cobalt is a naturally occurring element found in rocks, soil, water, plants, and animals. It is an essential micronutrient required for the growth of both plants and animals. Cobalt can be beneficial for humans because it is part of the Vitamin B₁₂. However, exposure to a high level of cobalt is harmful and can result in lung and heart effects and dermatitis.¹ Copper and nickel combined with other elements occur naturally in the earth's crust. Copper is an essential nutrient, while nickel has no known beneficial health effects. However, both metals may be harmful if ingested in excessive amounts. The main route of intake for these elements is from foods. Copper and nickel can be present in foods naturally, as a result of pollution, or from the storage and processing of foods.² Studies for cobalt, nickel and copper determination in water and biological matrices are very important because it is a good tool for environmental and toxicological monitoring.³⁻⁵ In spite of great improvements in the sensitivity and selectivity of modern instruments such as inductively coupled plasma mass spectrometry (ICP-MS), inductively coupled plasma optical emission spectroscopy (ICP OES) and electrothermal atomic absorption spectrometry (ETAAS), difficulties remain in the analysis of trace amounts of metals because of their low abundance levels in samples and the high complexity of sample matrices.^{6,7} Thus, efficient preconcentration and separation steps prior to their measurement remain essential. Various techniques have been devised for simultaneous separation and preconcentration of metal ions including liquid-liquid extraction,^{8,9} solid-phase extraction (SPE),¹⁰⁻¹² Hollow fiber liquid phase microextraction (HF-LPME),¹³ solidified floating organic drop microextraction (SFODME)¹⁴ and dispersive liquid-liquid microextraction (DLLME).^{15,16} The main objective of a sample preparation step is to isolate and concentrate the analytes of interest from the matrix and provide a suitable sample extract for instrumental determination. Liquid-liquid extraction (LLE) is a versatile classical sample preparation technique prescribed in many standard analytical methods. However, conventional LLE uses large amounts of potentially toxic organic solvents which are often hazardous and expensive. LLE is also considered to be a time consuming, tedious, and multistage operation.¹⁷ Efforts to overcome these limitations have

led to the development of microextraction in analytical chemistry.¹⁸ Miniaturized LLE or liquid phase microextraction (LPME) was introduced in 1996^{18,19} allowing the emergence of a different mode of LPME.^{17,20} Among different liquid phase microextraction techniques, dispersive liquid-liquid microextraction based on solidification of floating organic drop has attracted much research attention.^{17,21-25} This is due to its advantages of simplicity, rapidity, low cost, simple apparatus and consumption of very small amounts of low toxic organic solvent. This technique is based on the principle of DLLME and SFODME. Thus, a mixture of extraction (with a density lower than water) and dispersive solvent is rapidly injected into the aqueous sample containing the analyte of interest; a cloudy solution is formed and equilibrium is reached quickly due to the large surface area between the extraction solvent and the aqueous sample. The mixture is then centrifuged and the droplet of organic phase is floated on the aqueous phase. The sample vial is then placed in an ice bath, the drop is solidified, then easily removed and allowed to melt for determination. The solvent used in DLLME-SFO is similar to the solvent used in SFODME, i.e. it must have a density lower than water and a melting point close to room temperature (10-30 °C). Furthermore, the toxicity of the solvent of DLLME-SFO is lower than that of DLLME and there is no need for specific glass tubes.

In this study, the possibility of simultaneous enrichment of metal ions by DLLME-SFO was considered. Sodium diethyldithiocarbamate (DDTC), the classical organic reagent was selected as the complexing agent and a DLLME-SFO method combined with graphite furnace atomic absorption spectrometry (GFAAS) was developed for separation, enrichment and determination of cobalt, nickel and copper in water samples. Factors affecting the extraction efficiency and determination of the mentioned metal ions were systematically investigated.

EXPERIMENTAL

Reagents and chemicals

All reagents used were at least of analytical reagent grade and purchased from the Merck Company (Darmstadt, Germany). Deionized water was used throughout this study. The standard stock solutions of nickel (II) (1000 mg L^{-1}), cobalt (II) (1000 mg L^{-1}) and copper

*e-mail: sdadfarnia@yazduni.ac.ir

(II) (1000 mg L^{-1}) were prepared by dissolving the proper amount of $\text{Ni}(\text{NO}_3)_2 \cdot 6\text{H}_2\text{O}$ (Merck), CoCl_2 (Merck) and $\text{Cu}(\text{NO}_3)_2 \cdot 6\text{H}_2\text{O}$ (Merck) in 1% nitric acid solution. Standard solutions were prepared daily by appropriate dilution of stock solutions. 1-Undecanol was obtained from Merck (Darmstadt, Germany) and was used as the extracting solvent. Sodium chloride (Merck, Darmstadt, Germany) was of the highest purity available. A solution of Sodium diethyldithiocarbamate (DDTC, 0.1 mol L^{-1}) was prepared by dissolving the proper amount of DDTC in water.

Instrumentation


A Varian Zeeman spectra atomic absorption spectrometer, model 220Z was used for all metal measurements throughout this study. Varian spectra-AA hollow cathode lamps for Ni, Co and Cu were used as light sources and operated at currents of 4, 7 and 4 mA, a wavelength of 232.2, 342.5 and 327.4 nm with a spectra bandwidth of 0.2, 0.2 and 0.5 nm, respectively, as recommended by the manufacturers. The furnace tube was a standard platform tube with a pyrolytic coating. The furnace programs were optimized and are given in Table 1. Peak height measurement was used for all quantifications. The pH measurements were carried out with a Metrohm pH meter (model 691, Switzerland) using a combined glass calomel electrode. A centrifuge (Hitachi, Universal 320, Tuttlingen, Germany) was used for centrifuging.

Extraction procedure

The ionic strength and pH of a standard or sample solution were adjusted to 0.01 (using NaCl) and ~ 7 (using diluted nitric acid or ammonium hydroxide solution), respectively. Subsequently, 10 mL of solution containing no more than 1, 1.2 and 1.5 ng of copper, cobalt and nickel, respectively was placed into a $\sim 12 \text{ mL}$ vial and $100 \mu\text{L}$ of $1.3 \times 10^{-3} \text{ mol L}^{-1}$ of DDTC solution as complexing agent was added. The metal ions in the aqueous phase were complexed with DDTC. A mixture of $100 \mu\text{L}$ 1-undecanol (as the extraction solvent) and $200 \mu\text{L}$ acetone (as the dispersive solvent) was then rapidly injected into the aqueous sample. In this stage, a cloudy solution was formed in the vial which was stable for a long period and complexes were extracted into 1-undecanol within a few seconds. The mixture was then centrifuged at 2200 rpm for 3 min and the dispersed droplets of extraction solvent were coagulated and floated on the top of the aqueous phase. The vial was transferred into a beaker containing crushed ice and the organic solvent containing the analyte complexes was solidified after 5 min. The solidified extract was then transferred into a conical vial where it melted immediately. Finally, for determination of each analyte, $10 \mu\text{L}$ of the extract was manually injected into the graphite furnace atomic absorption spectrometer.

RESULTS AND DISCUSSION

Sodium diethyldithiocarbamate (DDTC) is a classical ligand that forms complexes with many metal ions including Cu^{2+} , Co^{2+} and Ni^{2+} , according to Equation 1:



DDTC is relatively soluble in water but its complexes have low solubility in aqueous phase. In the preliminary experiments, it was observed that the metal complexes of DDTC are soluble in 1-undecanol, hence DDTC was used for the separation and extraction of Ni, Co,

and Cu by the DLLME-SFO method followed by their determination by GFAAS as a micro amount sample analysis technique.

In order to obtain a high enrichment factor, different parameters affecting the complex formation, extraction and analyte determination were optimized using the univariable approach.

Optimization of furnace temperature program

At the primary step of this analysis, it was demonstrated that the temperature program suggested by manufacturers would not be efficient in this method as the magnitude of background was high. In order to avoid the loss of the metal ions of interest and in order to eliminate the background signal during the analysis, the temperature of the ETAAS was optimized and results are provided in Table 1. Under these conditions, the background was low and the peaks had a normal shape. With regard to the boiling point of 1-undecanol ($243 \text{ }^\circ\text{C}$), it was proven that a drying temperature of $270 \text{ }^\circ\text{C}$ with the hold time of 10 s is necessary for the evaporation of the solvent. The optimal pyrolysis temperature for these metals was $900 \text{ }^\circ\text{C}$ and the optimal atomization temperatures were, 2600, 2500 and $2600 \text{ }^\circ\text{C}$ for Cu^{2+} , Co^{2+} and Ni^{2+} , respectively (Figure 1). Under these conditions no modifiers were required and the proper results were achieved.

Table 1. Temperature program of EtAAS for determination of analytes

Steps	Temperature ($^\circ\text{C}$)			Time (S)	Argon flow rate (L min^{-1})
	Ni	Co	Cu		
1	95	95	95	5	3
2	120	120	120	40	3
3	270	270	270	10	3
4	800	800	800	10	3
5	2600	2500	2600	3.1	0
6	2600	2500	2600	2	3

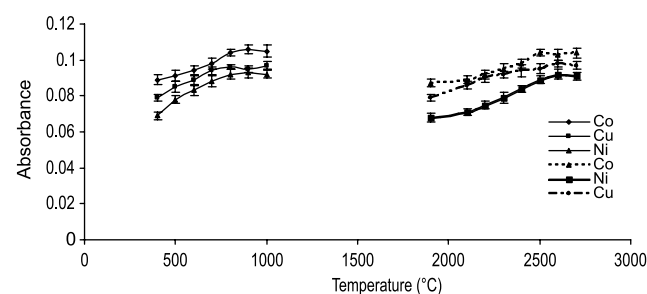


Figure 1. Effect of pyrolysis and atomization temperature on the absorption of $10 \mu\text{g L}^{-1}$ of Ni, Co and Cu

Selection of nature of organic and dispersive solvent

In the DLLME-SFO procedure, the selection of organic solvent has a significant effect on the recovery factors of the metal ion complexes. The extracting solvent must fulfill several requirements as follows: 1- It must be immiscible in the water and miscible with the disperser solvent. 2 - Its melting point should be near room temperature ($10\text{-}30 \text{ }^\circ\text{C}$). 3 - Its density must be less than water. 4 - The complexes should have high solubility in extracting solvent and the solvent must be compatible with the analytical technique of measurement. 5 -It must have low volatility in order to be stable during the extraction period.

Thus, several extraction solvents usually used in SFODME including 1-undecanol, 1-dodecanol, 1,10-dichlorodecane and n-hexadecane were investigated. Among these solvents, 1-undecanol was selected as

the extraction solvent since it afforded the best extraction efficiency. The extraction efficiency of 1-dodecanol was around 89% of 1-undecanol. However, n-hexadecane and 1,10-dichlorodecane were ruled out as n-hexadecane does not have sufficient solubility in usual dispersive solvents while 1,10-dichlorodecane produced high background during the analysis, interfering with the determination of the analytes.

The disperser solvent must be miscible with extraction solvent and water. Thus, in this experiment acetone, ethanol, methanol and acetonitrile were tested. With acetonitrile, emulsion was formed and separation of the two phases proved difficult. With acetone on the other hand, the cloud was very stable and recoveries higher than with either, ethanol or methanol. Thus, acetone was selected as the most suitable dispersive solvent due to its low toxicity, low cost and high analytical signals.

Effects of volume of extraction and disperser solvent

Demonstration of the preconcentration capability of the DLLME-SFO system is an important aspect of the method development. An increase in the ratio of volume of aqueous phase to organic phase will increase the preconcentration factor, but it may reduce the extraction efficiency in a given extraction time. The influence of 1-undecanol volume (20-160 μL) on extraction efficiency was investigated. Several experiments were performed using 200 μL of acetone as disperser solvent and different volumes of 1-undecanol as the extraction solvent. The relative recoveries indicate that when the volume of 1-undecanol is varied in the range of 30-160 μL , extraction efficiency is maximal and constant. Therefore, a volume of 100 μL of 1-undecanol was used for optimization (for each extract, the determination of each analyte was repeated three times), whereas 30 μL of 1-undecanol was used when obtaining the performance data and analyzing the real sample

The effects of the volume of acetone as the dispersive solvent in the 50-400 μL range on the extraction efficiency of analytes were examined while the volume of 1-undecanol as the extraction solvent was fixed at 100 μL . The results showed that by increasing the volume of disperser solvent up to 200 μL , the absorbance of analytes increased and then leveled off up to a volume of 300 μL of acetone. When the volume of acetone was low, 1-undecanol was not completely dispersed and extraction efficiency was low. At a volume of acetone greater than 300 μL , the extraction efficiency was slightly decreased probably due to the increase in the solubility of the analytes in the aqueous phase containing a high percentage of acetone. Thus, 200 μL of acetone was selected as the optimal volume of the dispersive solvent.

Effect of sample pH

The pH of the sample solution is one of the most important factors affecting the formation of the complexes and their subsequent extraction into organic phase. The effect of pH of solution on the extraction of DDTc complexes of copper, cobalt and nickel was studied by varying the pH within the range 0.5-11. The pH was adjusted by either diluted nitric acid or ammonium hydroxide solution, while the other variables were kept constant. The results illustrated in Figure 2 demonstrate that at a pH>6 the analytical signal is almost constant. The progressive decrease in extraction at pH<6 might be due to the competition of the proton with the analytes for the reaction with DDTc. Therefore, a pH~7 was selected as the optimum pH for the subsequent work.

Effect of DDTc concentration

The efficiency of analyte extraction is dependent on the quantitative formation of the complex between the ligand and the analytes.

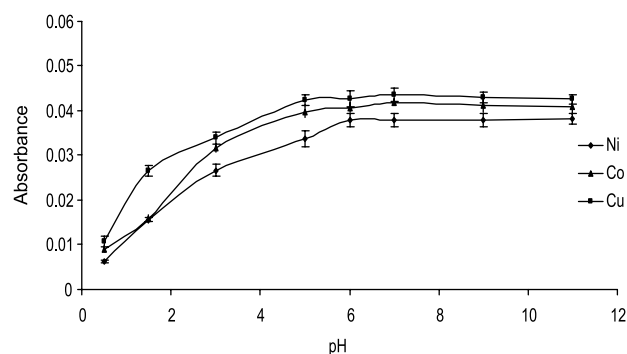


Figure 2. Effect of pH on the extraction of analytes by DLLME-SFO. Extraction conditions: sample volume, 10 mL; analytes concentration, 50 ng L⁻¹; volume of organic phase, 100 μL ; acetone volume, 200 μL ; DDTc concentration 3×10^{-7} mol L⁻¹; salt concentration 5×10^{-3} mol L⁻¹

At constant aqueous phase pH, up to a certain amount of ligand, formation of the complex and consequently the extraction efficiency, increases according to the increase in ligand concentration while extraction efficiency remains constant at higher concentrations of ligand. Thus, the effect of DDTc concentration on the extraction efficiency was evaluated by varying its concentration in the range of 1.6×10^{-8} - 3.4×10^{-7} mol L⁻¹. The analyte signals reached their maximum when the concentration of DDTc was 1.3×10^{-7} mol L⁻¹ and leveled off at higher concentrations (Figure 3). Therefore, a concentration of 1.3×10^{-7} mol L⁻¹ of DDTc was selected as the optimum concentration for further studies.

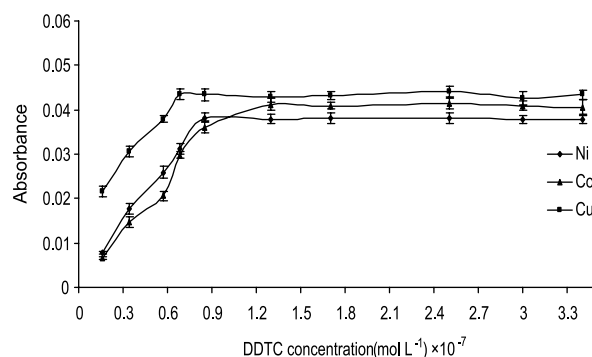


Figure 3. Effect of concentration of DDTc on the extraction of analytes by DLLME-SFO. Extraction condition: sample volume, 10 mL; analytes concentration, 50 ng L⁻¹; volume of organic phase, 100 μL ; acetone volume, 200 μL ; pH ~7; salt concentration 5×10^{-3} mol L⁻¹

Effect of salt

To study the effect of salt addition on extraction efficiency, the concentration of NaCl was changed in the range 0.0-0.1 mol L⁻¹ while other experimental parameters were kept constant. Addition of salt to the aqueous phase usually results in an improvement of extraction efficiency by the process of the salting-out effect. The results indicated a gradual increase in the analytical signals of the metal ions with increased NaCl concentrations up to 0.01 mol L⁻¹ which then remained constant with further increases in the salt concentration. Thus, a concentration of 0.01 mol L⁻¹ of NaCl was used for further studies.

Effect of sample volume

In order to explore the possibility of enriching low concentrations

of the analytes from the large volume, the effect of sample volume on extraction of 0.5 ng of analytes from different aqueous volumes (5-50 mL) at optimum conditions was examined using an appropriate size vial. The results presented in Figure 4 showed that extraction efficiencies were constant up to a volume of 40 mL and then decreased upon further increase in sample volume. However, as ETAAS has good sensitivity, a more convenient sample volume of 10 mL was used in further experiments. Based on the organic phase volume of 30 μ L and sample volume of 10 mL, a preconcentration factor of 333 was determined. Extending the sample processing volume, however, improved method sensitivity. In the present study, the preconcentration factor can be extended by increasing the sample volume to 40 mL.

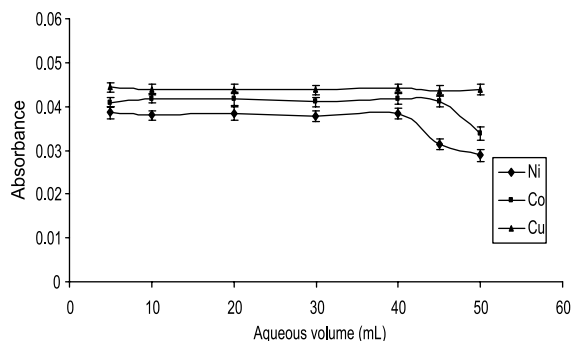


Figure 4. Effect of sample volume on extraction of analytes by DLLME-SFO. Extraction condition: pH ~7; analytes concentration, 50 ng L⁻¹; volume of organic phase, 100 μ L; acetone volume, 200 μ L; DDTC concentration 3 \times 10⁻² mol L⁻¹; salt concentration 5 \times 10⁻³ mol L⁻¹

Effect of extraction time

In DLLME-SFO, extraction time is defined as the time interval between the time of injection of the mixture of dispersive and extraction solvent and the time of centrifugation. The effects of the extraction time on the analytical signals were examined over the time range of 0-10 min under constant experimental conditions. The results showed that the extraction time had no significant impact on extraction efficiency. This can be explained on the bases that after the formation of a cloudy solution, the surface area between the extraction solvent and the aqueous phase is very large. The transition of the complex from aqueous phase to the extraction solvent and achievement of equilibrium is therefore fast. Thus, the most important advantage of the DLLME-SFO method is its time independency. In this method, the time-consuming steps are centrifuging of the sample solution and solidification of 1-undecanol, which together take about 8 min.

Effect of diverse ions

The effect of potential ions usually present in natural water on the preconcentration and determination of analytes was examined. For this purpose, a solution of 50 ng L⁻¹ of the analytes containing various amounts of interfering ions was treated according to the optimized procedure. The tolerance limit of coexisting ions was defined as the largest amount producing a variation of less than 5% in the recovery of analytes. The tolerance limits of diverse ions are given in Table 2. The results indicated that the presence of the ions at the mole ratio shown in Table 2 has no significant effect on the extraction of analytes.

Figures of merit of the proposed method

The performance characteristics of the method were obtained by processing 10 mL of standard solution of the analytes under the

Table 2. Tolerance limit of diverse ions on the quantitative recovery of analytes (analytes concentration 50 ng L⁻¹)

Ions	Mole ratio (Ion/analytes)
K ⁺ , Mg ²⁺ , Ca ²⁺ , Al ³⁺ , I ⁻ , F ⁻ , Br ⁻ , SO ₄ ²⁻ , CO ₃ ²⁻	1000
Hg ²⁺ , Zn ²⁺ , Fe ³⁺ , Pb ²⁺	750
Cd ²⁺	500

optimized conditions. The calibration graphs exhibited linearity over the 10-120 ng L⁻¹ range for nickel, 10-100 ng L⁻¹ for cobalt and 7-150 ng L⁻¹ for copper. The equations of the calibration curves and correlation coefficients for Ni²⁺, Co²⁺ and Cu²⁺ were: A = 0.0025C + 0.004 (R² = 0.9997), A = 0.0027C + 0.0061 (R² = 0.9998) and A = 0.003C - 0.0029 (R² = 0.9993), respectively. The enhancement factors, defined as the ratio of the slope of calibration curves prepared from aqueous solutions submitted to the recommended procedure to that obtained without preconcentration, were found to be 277 for Ni²⁺, 270 for Co²⁺ and 300 for Cu²⁺.

The limits of detection, defined as 3S_b/m (where S_b is standard deviation of the blank and m is the slope of the calibration graph) were 1.2, 1.1, 1.0 ng L⁻¹, limits of quantification, defined as 10S_b/m were 3.9, 3.7, 3.4 ng L⁻¹, and relative standard deviation (RSD) for 7 replicate measurements at 40 ng L⁻¹, were 3.2%, 4.4%, 3.8% for Ni²⁺, Co²⁺ and for Cu²⁺, respectively.

Application

To examine the accuracy of the proposed procedure, the method was applied to the determination of analytes in tap water, well water, spring water, river water and sea water. The water samples were filtered through a 0.45 μ m pore-size Millipore membrane and were treated according to the recommended procedure. The accuracy of the method was verified by the analysis of the samples spiked with known amounts of the analytes. As demonstrated in Table 3, the recoveries of spiked samples were good (95.5-103.5%). Thus, these results indicate that the matrices of tap, well, spring, river and sea have no significant effect on the DLLME-SFO-ETAAS method for the determination of the analytes.

Furthermore, in order to verify the accuracy of the proposed method, the procedure was used for the determination of Co, Ni and Cu in certified sea water (NASS-1). The concentrations of cobalt, copper and nickel in the sample were found to be 4.1 \pm 0.4, 98 \pm 5 and 259 \pm 10 ng L⁻¹, respectively, which at a 95% confidence limit, are in good agreement with the certified values (ng L⁻¹) of 4 \pm 1 for Co, 99 \pm 10 for Cu and 257.0 \pm 27 for Ni. Thus, the method is reliable for determination of Co, Cu and Ni in natural water samples.

Comparison with other methods

Separation and determination of analytes in water samples by the developed DLLME-SFO method was compared with that of other reported liquid microextraction methods and results shown in Table 4. With the exception of SFODME-GFAAS and IL-SDME-LTEV-ICP-MS, the proposed DLLME-SFO method has a higher enrichment factor and consequently a lower detection limit. However, the extraction time of the proposed method is shorter than that of SFODME-GFAAS.

CONCLUSIONS

It has been demonstrated that the DLLME-SFO method can be used for simultaneous separation and enrichment of ultra-traces of

Table 3. Determination of analytes in real water samples

Sample	Added (ng L ⁻¹)			Found ^a (ng L ⁻¹)			Recovery (%)		
	Ni	Co	Cu	Ni	Co	Cu	Ni	Co	Cu
Tap water	0	0	0	88.9 ± 2.4	75.8 ± 2.2	79.9 ± 2.6	-	-	-
	20	20	20	108.5 ± 2.8	95.1 ± 1.6	99.7 ± 3.8	98.0	96.5	99.0
Well water	0	0	0	98.2 ± 2.4	83.8 ± 2.3	110.2 ± 3.4	-	-	-
	20	20	20	117.9 ± 2.7	102.9 ± 2.9	129.9 ± 3.4	98.5	95.5	98.5
Spring water	0	0	0	44.3 ± 1.2	56.1 ± 2.3	35.4 ± 1.2	-	-	-
	20	20	20	64.4 ± 1.7	75.9 ± 3.1	54.7 ± 1.3	100.5	99.0	96.5
River water*	0	0	0	154.9 ± 5.2	163.6 ± 5.9	147.2 ± 6.3	-	-	-
	20	20	20	175.1 ± 8.2	183.4 ± 7.3	167.9 ± 5.2	101.0	99.0	103.5
Sea water*	0	0	0	300.0 ± 7.8	254.4 ± 6.8	390.0 ± 8.1	-	-	-
	20	20	20	319.6 ± 7.1	273.8 ± 7.4	409.1 ± 9.2	98.0	97.0	95.5

^a Mean and standard deviation of three determinations. *4 mL of the sample was diluted to the 10 mL.

Table 4. Comparison of enrichment, detection limit and sample volume of the proposed method with others reported microextraction methods

Method	Enrichment factor			Detection limit (ng L ⁻¹)			Sample volume (mL)	Refs.
	Ni	Co	Cu	Ni	Co	Cu		
CPE-ETAAS	46	53	53	9	8	6	10	31
CPE-ETAAS	27	-	-	120	-	-	10	30
SDME-LTEV-ICP-MS	-	125.0	-	-	0.99 (pg L ⁻¹)	-	1	26
HF-LPME-ETV-ICP-MS	-	-	305.0	-	-	12.4	2.5	27
DLLME-FO-LADS	-	165.0	-	-	200.0	-	10	16
DLLME-FAAS	-	-	42.0	-	-	3000.0	5	28
IL-SDME-ETV-ICP-MS	-	350.0	-	-	1.5	-	1.5	29
DLLME-ETAAS	101.0	200.0	-	21.0	33.0	-	10	32
SFODME-ETAAS	490.0	500.0	-	0.3	0.4	-	10	14
HF-LPME-ETAAS	60.0	-	-	30.0	-	-	3	13
DLLME-SFO-ICP-OES	-	76.0	93.0	-	200.0	200.0	20	24
DLLME-SFO-ETAAS	277.0	270.0	300.0	1.2	1.1	1.1	10	This work

cobalt, nickel and copper. Furthermore, the method permits effective separation and preconcentration of analytes and final determination by ETAAS in several categories of natural waters. The most important advantages of the method are very short extraction time, ease of operation, minimum consumption of low toxic organic solvent, and a high enrichment factor.

REFERENCES

- Sasmaz, A.; Yaman, M.; *Soil Sci. Plan. Anal.* **2006**, *37*, 1845.
- Soylak, M.; Elci, L.; Dogan, M.; *Anal. Lett.* **1997**, *30*, 623.
- Soylak, M.; Elci, L.; Narin, I.; Dogan, M.; *Trace Elem. Elettroly.* **2001**, *18*, 26.
- Mckenzie, H. A.; Smythe, L. E.; *Quantitative Trace Analysis of Biological Materials*, Elsevier: Amsterdam, 1988.
- Baird, C.; *Environmental Chemistry*, 2nd ed., Freeman and Longman: UK, 1999.
- Narin, I.; Soylok, M.; *Talanta* **2003**, *60*, 215.
- Dadfarnia, S.; McLeod, C. W.; *Appl. Spectrosc.* **1994**, *48*, 1331.
- Rao, T. P.; Metilda, P.; Gladis, J. M.; *Crit. Rev. Anal. Chem.* **2005**, *35*, 247.
- Oliva, A.; Molinari, A.; Zuniga, F.; Ponce, P.; *Microchim. Acta* **2002**, *140*, 201.
- Hejazi, L.; Mohammadi, D. E.; Yamini, Y.; Brereton, R. G.; *Talanta* **2004**, *62*, 183.
- Rekha, D.; Suvardhan, K.; Dilip Kumar, J.; Subramanyam, P.; Reddy Prasad, P.; Lingappa, Y.; Chiranjeevi, P.; *J. Hazard. Mater.* **2007**, *146*, 131.
- Ghaedi, M.; Ahmadi, F.; Shokrollahi, A.; *J. Hazard. Mater.* **2007**, *142*, 272.
- Abulhassani, J.; Manzoori, J. L.; Amjadi, M.; *J. Hazard. Mater.* **2010**, *176*, 481.
- Shirani Bidabadi, M.; Dadfarnia, S.; Haji Shabani, A. M.; *J. Hazard. Mater.* **2009**, *166*, 291.
- Afzali, D.; Ghazizadeh, A.; Salari, H.; *Quim. Nova* **2011**, *34*, 1124.
- Mohammadi, S. Z.; Baghelani, Y. M.; Mansori, F.; Shamspur, T.; Afzali, D.; *Quim. Nova* **2012**, *35*, 198.
- Dadfarnia, S.; Haji Shabani, A. M.; *Anal. Chim. Acta* **2010**, *658*, 107.
- Jeannot, M. A.; Cantwell, F. F.; *Anal. Chem.* **1996**, *68*, 2236.
- He, Y.; Lee, H. K.; *Anal. Chem.* **1997**, *69*, 4634.
- Pereira, F. P.; Lavilla, I.; Bendicho, C.; *Spectrochim. Acta, Part B* **2009**, *64*, 1.
- Asadollahi, T.; Dadfarnia, S.; Haji Shabani, A. M.; *Talanta* **2010**, *82*, 208.
- Leong, M. I.; Huang, Sh. Da.; *J. Chromatogr. A* **2008**, *1211*, 8.
- Xu, H.; Ding, Z. Q.; Lv, L. L.; Song, D. D.; Feng, Y. Q.; *Anal. Chim. Acta* **2009**, *636*, 28.

24. Yamini, Y.; Rezaee, M.; Khanchi, A.; Faraji, M.; Saleh, A., *J. Chromatogr. A* **2010**, *1217*, 2358.
25. Rohani Moghadam, M.; Haji Shabani, A. M.; Dadfarnia, S.; *J. Hazard. Mater* **2011**, *197*, 176.
26. Xia, L.; Hu, B.; Jiang Z.; Wu Y.; Liang, Y.; *Anal. Chem.* **2004**, *76*, 2910.
27. Xia, L.; Wu, Y.; Hu, B.; *J. Mass Spectrom.* **2007**, *42*, 803.
28. Frajzadeh, M. A.; Venkateswarana, P.; Seal, L.; *J. Ind. Eng. Chem.* **2007**, *14*, 110.
29. Xia, L.; Hi, X.; Wu Y.; Hu, B.; Chen, R.; *Spectrochim. Acta, Part B* **2008**, *63*, 1290.
30. Sun, Zh.; Liang, P.; Ding, Q.; Cao, J.; *J. Hazard. Mater.* **2006**, *137*, 943.
31. Meeravali, N. N.; Reddy, M. A.; Kumar, S. J.; *Anal. Sci.* **2007**, *23*, 351.
32. Jiang, H.; Qin, Y.; Hu, B.; *Talanta* **2008**, *74*, 1160.